



Digital Blood Pressure Monitor

Model UA-767F

Instruction Manual *Original*

Manuel d'instructions *Traduction*

Manual de Instrucciones *Traducción*

Manuale di Istruzioni *Traduzione*

Instructiehandleiding *Vertaling*

Bruksanvisning *Översättning*

Ohjekirja *Käännös*

Instrukcja obsługi *Tłumaczenie*

使用手冊 *翻譯*

ترجمہ دليل الإستعمال

English

Français

Español

Italiano

Nederlands

Svenska

Suomi

Polski

中文

عربي

1WMPD4005014A

Issued Date: 19 Aug. 2025

Contents

Dear Customers.....	2
Preliminary Remarks	2
Intended Purpose	2
Clinical Benefit.....	2
Precautions.....	2
Parts Identification	5
Symbols.....	6
Operation Mode	9
Using the Monitor.....	11
Inserting / Changing the Batteries.....	11
Connecting the Air Hose	12
Connecting the AC Adapter	12
Adjusting the Built-in Clock	13
Selecting the Correct Cuff Size	14
Applying the Arm Cuff	14
How to Take Accurate Measurements	16
Measurement	16
After Measurement.....	16
Measurements	17
Normal Measurement.....	17
Measurement with the Desired Systolic Blood Pressure.....	18
Notes for Accurate Measurement	18
Recalling the Memory Data	19
What Is The IHB/AFib Indicator?	21
What Is The AFib?	21
%IHB/AFib.....	21
Pressure Bar Indicator	22
WHO Classification Indicator	22
About Blood Pressure.....	23
What is Blood Pressure?.....	23
What is Hypertension and How is it Controlled?	23
Why Measure Blood Pressure at Home?	23
WHO Blood Pressure Classification.....	23
Blood Pressure Variations.....	23
Troubleshooting	24
Maintenance	25
Technical Data.....	25

Dear Customers

Thank you for purchasing a state-of-the-art A&D blood pressure monitor. Designed for ease of use and accuracy, this device will facilitate your daily blood pressure regimen.

We recommend that you read through this manual carefully before using the device for the first time.

Preliminary Remarks

- ☐ This device conforms to the Medical Device Regulations (EU 2017/745) and UKCA Medical Device Regulations 2002 for Medical Products. This is made evident by the CE2797 and UKCA0086 mark of conformity. (2797 and 0086: The reference numbers to the involved notified body.)
- ☐ The device is designed for use by people 13 years and older, not newborns or infants.
- ☐ This device fulfils the following provisions.

CE₂₇₉₇ **Medical Device Regulation (EU 2017/745)**

UK
CA₀₀₈₆ **UKCA Medical Devices Regulations 2002**

Intended Purpose

The UA-767F Digital Blood Pressure Monitor is intended to be used by patients to measure systolic and diastolic blood pressure and pulse rate in the home environment. The UA-767F provides the patient with an indication of an irregular heartbeat allowing further medical attention to be sort.

Clinical Benefit

Successful assessment of blood pressure reading in accordance with the device's intended purpose.

Precautions

- ☐ Precision components are used in the construction of this device. Extremes in temperature, humidity, direct sunlight, shock or dust should be avoided.
- ☐ Clean the device and cuff with a dry, soft cloth or a cloth dampened with water and a neutral detergent. Never use alcohol, benzine, thinner or other harsh chemicals to clean the device or cuff.

- ☐ Avoid tightly folding the cuff or storing the hose tightly twisted for long periods, as such treatment may shorten the life of the components.
- ☐ Take care to avoid accidental strangulation of babies or infants with the hose and cable.
- ☐ Do not twist the air hose during the measurement. This may cause injury due to continuous cuff pressure.
- ☐ The device and cuff are not water resistant. Prevent rain, sweat and water from damaging the device and cuff.
- ☐ Measurements may be distorted if the device is used close to televisions, microwave ovens, cellular telephones, X-ray or other devices with strong electrical fields.
- ☐ Wireless communication devices, such as home networking devices, mobile phones, cordless phones and their base stations, and walkie-talkies can affect this blood pressure monitor.
Therefore, a minimum distance of 30 cm should be kept from such devices.
- ☐ When reusing the device, confirm that the device is clean.
- ☐ Used equipment, parts and batteries are not treated as ordinary household waste, and must be disposed of according to the applicable local regulations.
- ☐ When the AC adapter is used, make sure that the AC adapter can be readily removed from the electrical outlet when necessary.
- ☐ Do not modify the device. It may cause accidents or damage to the device.
- ☐ To measure blood pressure, the arm must be squeezed by the cuff hard enough to temporarily stop blood flow through the artery. This may cause pain, numbness or a temporary red mark to the arm. This condition will appear especially when measurement is repeated successively. Any pain, numbness, or red marks will disappear with time.
- ☐ Measuring blood pressure too frequently may cause harm due to blood flow interference. Check that the operation of the device does not result in prolonged impairment of blood circulation, when using the device repeatedly.
- ☐ If you have had a mastectomy or lymph node clearance, please consult a doctor before using the device.
- ☐ Do not let children use the device by themselves and do not use the device in a place within the reach of infants. This may cause accidents or damage.
- ☐ There are small parts that may cause a choking hazard if swallowed by mistake by infants.
- ☐ Unplug the AC adapter when not in use during the measurement.
- ☐ Use of accessories not detailed in this manual may compromise safety.
- ☐ Should the battery short-circuit, it may become hot and potentially cause burns.
- ☐ Allow the device to adapt to the surrounding environment before use (about one hour).
- ☐ Clinical testing has not been conducted on newborn infants and pregnant

women. Do not use on newborn infants or pregnant women.


- ☐ Do not touch the batteries, the DC jack, and the patient at the same time. That may result in electrical shock.
- ☐ Do not inflate without wrapping the cuff around the upper arm.
- ☐ This is a medical device for use by layperson. Please consult your healthcare provider with any questions or concerns you may have regarding your condition.
- ☐ When any serious incident occurs in relation to this device, report to its manufacturer and the competent authority in your country.
- ☐ Confirm for proper operation before use, if the packaging is damaged, unintentionally opened and exposed to environmental conditions outside of those specified.
- ☐ This device is not intended to diagnose heart arrhythmias. If the Irregular Heart Beat indicator illuminates frequently and is unrelated to patient movement during blood pressure measurement, further medical attention must be sort.

Contraindications


The following are precautions for proper use of the device.

- ☐ Do not apply the cuff on an arm with another medical electrical equipment attached. The equipment may not function properly.
- ☐ People who have a severe circulatory deficit in the arm must consult a doctor before using the device, to avoid medical problems.
- ☐ Do not self-diagnose the measurement results and start treatment by yourself. Always consult your doctor for evaluation of the results and treatment.
- ☐ Do not apply the cuff on an arm with an unhealed wound.
- ☐ Do not apply the cuff on an arm receiving an intravenous drip or blood transfusion. It may cause injury or accidents.
- ☐ Do not use the device where flammable gases such as anesthetic gases are present. It may cause an explosion.
- ☐ Do not use the device in highly concentrated oxygen environments, such as a high-pressure oxygen chamber or an oxygen tent. It may cause a fire or explosion.
- ☐ Do not provide any servicing and perform maintenance while the medical device is in use.

Parts Identification


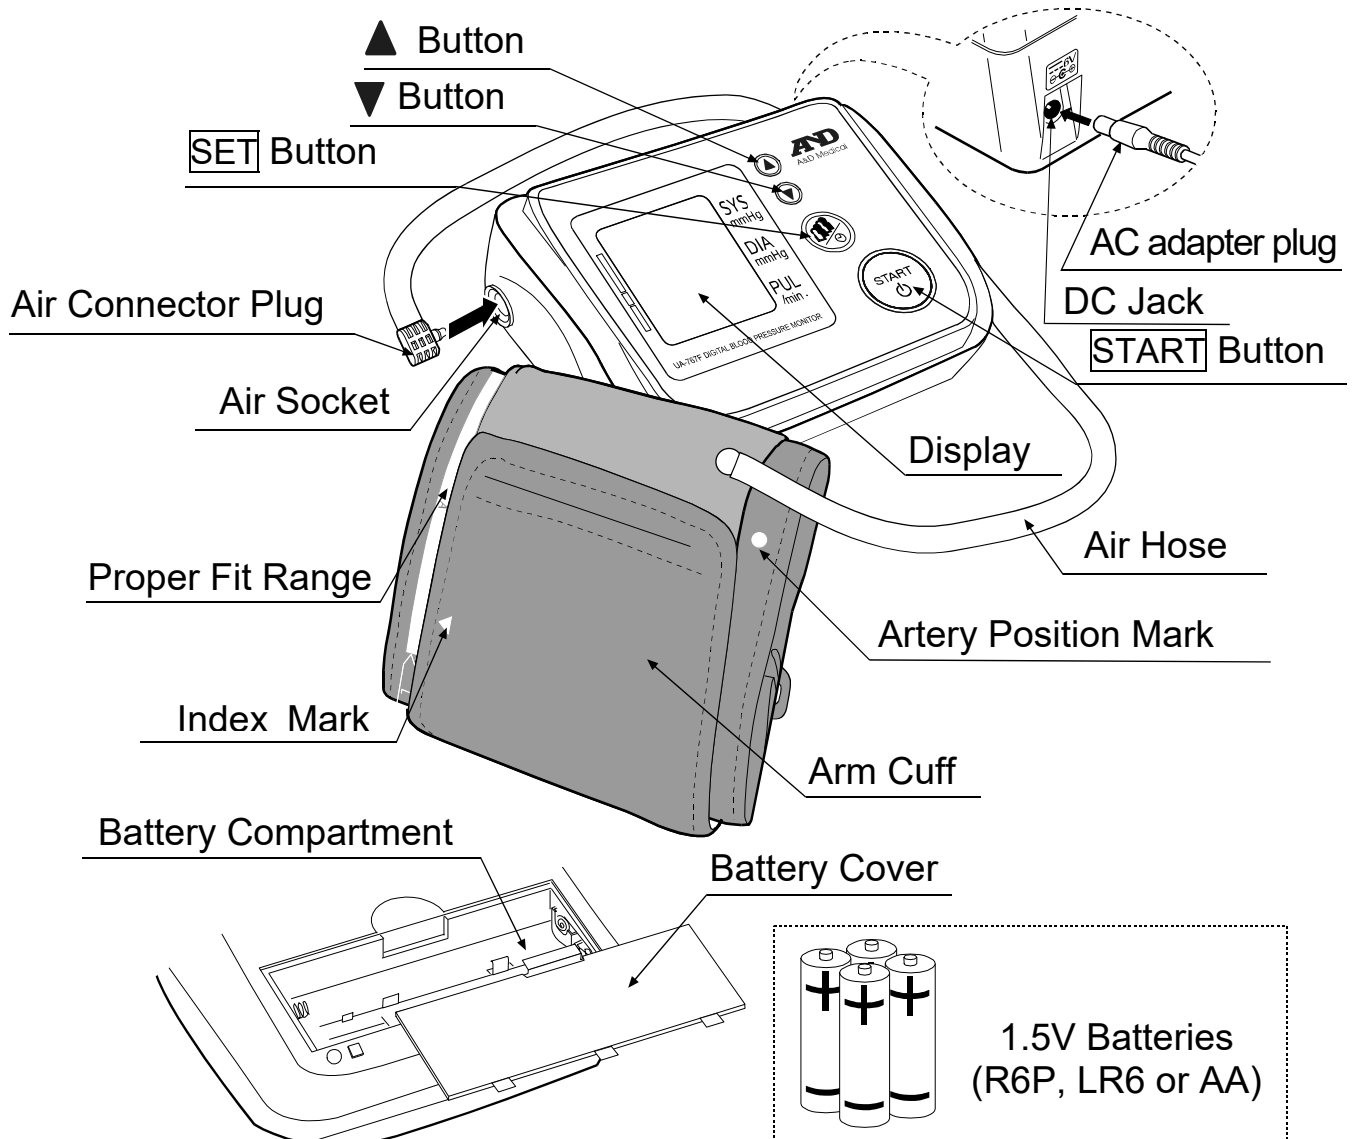


Display

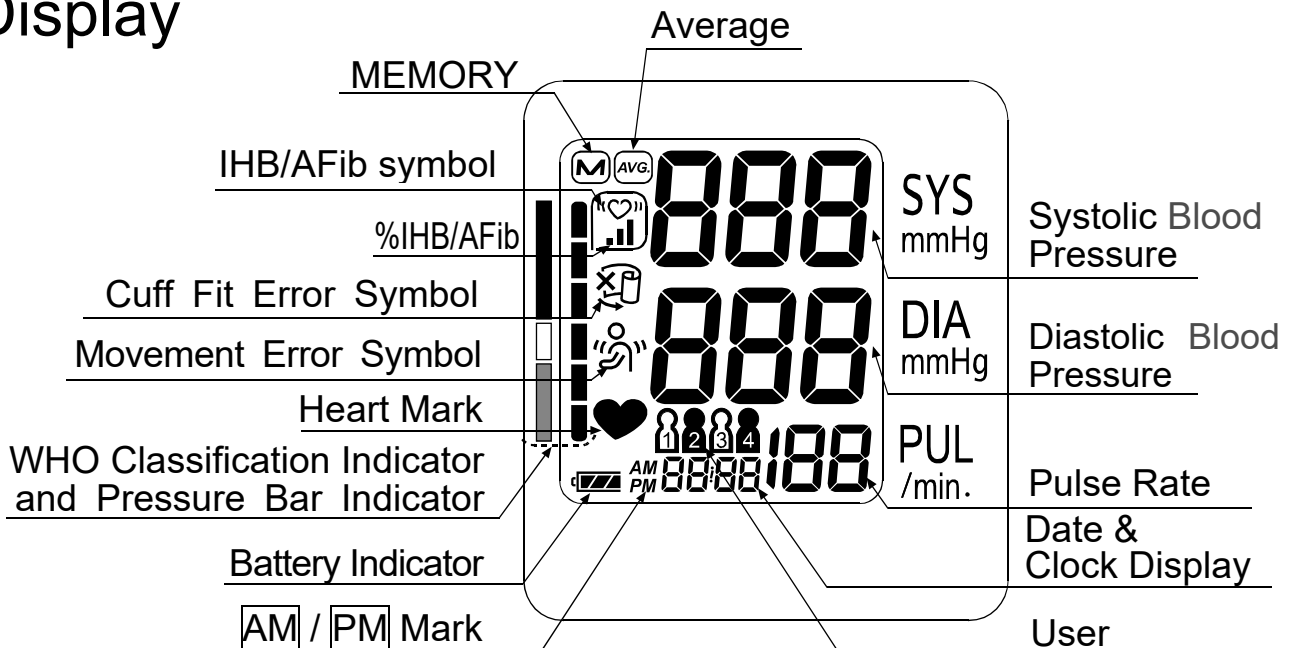

Symbols

The symbols that are printed on the device and the packaging.

Symbols	Function / Meaning
	Press  to turn on the device. Press  during measurement to enter standby.
SYS	Systolic blood pressure in mmHg
DIA	Diastolic blood pressure in mmHg
PUL	Pulse per minute
	Battery installation guide
	Direct current
	Type BF applied part
	CE marking
	European Authorized Representative
	UK Conformity Assessed marking
	UK Responsible Person
	Medical Device
	Manufacturer
	Date of manufacture
IP	International protection symbol
	WEEE label
	Serial Number
	Unique Device Identifier
	Refer to instruction manual/booklet *1
	Polarity of DC jack
	Keep dry
	Temperature limit
	Humidity limitation
	Atmospheric pressure limitation
	EU Importer
	UK Importer

*1 The symbol color: Blue



Symbols

Symbols that appear on the display

Symbols	Function / Meaning	Recommended Action
	Appears while measurement is in progress. It blinks when the pulse is detected.	Measurement is in progress. Remain as still as possible.
	IHB/AFib symbol Appears when an irregular heartbeat is detected. It may light when a very slight vibration like shivering or shaking is detected.	Apply the cuff correctly, then take another measurement. If the «  » symbol continues to appear, we recommend you to consult with your physician.
	Appears when a body or arm movement is detected.	The reading may yield an incorrect value. Take another measurement. Remain still during the measurement.
	 appears during the measurement when the cuff is attached loosely.	The reading may yield an incorrect value. Apply the cuff correctly, and take another measurement.
	Detected rate of IHB/AFib in memory $\% \text{IHB/AFib} = \frac{\left(\begin{array}{c} \text{Number of detected} \\ \text{IHB/AFibs in memory} \end{array} \right)}{\left(\begin{array}{c} \text{Total number} \end{array} \right)} \times 100 [\%]$	_____
	User	_____
	Displayed when the data in memory is displayed.	_____
	Average data	_____
	FULL BATTERY The battery power indicator during the measurement.	_____
	LOW BATTERY The battery is low when it blinks.	Replace all batteries with new ones when the mark blinks.

Symbols

Symbols that appear on the display

Symbols	Function / Meaning	Recommended Action
	Unstable blood pressure due to movement during the measurement.	Take another measurement. Remain very still during the measurement.
	The systolic and diastolic values are within 10 mmHg from each other.	Apply the cuff correctly, and take another measurement.
	The pressure value did not increase during the inflation.	
	The cuff is not applied correctly.	
	PUL DISPLAY ERROR The pulse is not detected correctly.	
	Blood pressure monitor internal error	Remove the batteries and press the START button, and then install the batteries again. If the error still appears, contact the dealer.
		
AM	Data taken between 4:00 and 9:59	_____
PM	Data taken between 18:00 and 1:59	_____

Operation Mode

1. Normal Measurement

Press the **START** button. Blood pressure is measured and the data is stored in memory. This device can store the last 60 measurements for each of the four users in memory.

2. Recalling the Data

Press the **▲** or **▼** button to recall the data in memory. The average of all measurements is displayed, as indicated in the figure at the right.


Then, each time the **▼** button is pressed, the memory data is displayed as follows.

Most recent data (No.n, in the example, No.35)




Last data (No.1)

For details on recalling the data, refer to the section "Recalling the Memory Data". (See page 19.)

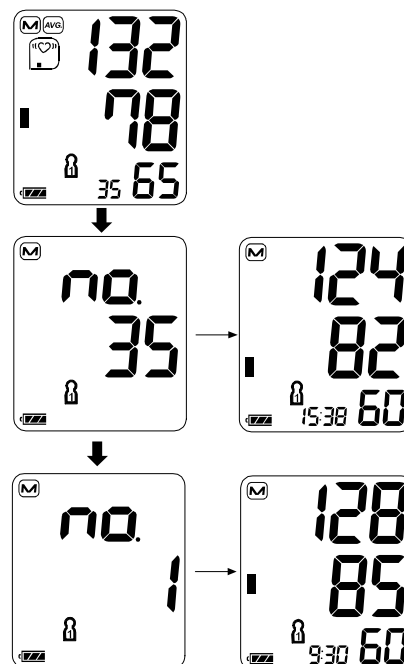

3. Changing user for memory display


Press the **SET** button while a memory is displayed. The user is changed, and the average of measurement values for that user is displayed.

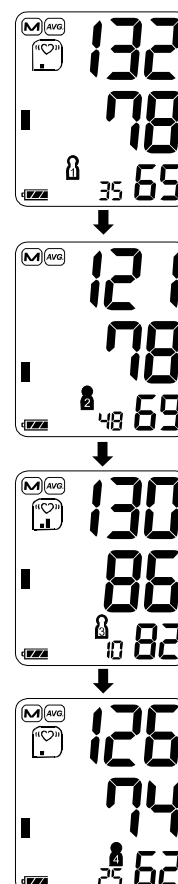

Operation Mode

4. Deleting Data Stored in Memory

In standby, press both the ▲ and ▼ buttons. The **M** mark, battery indicator and user mark will appear. When you would like to delete the memory data of the currently displayed user, press and hold both the ▲ and ▼ buttons until the illuminated **M** mark starts blinking.



5. Measurement with the Desired Systolic Blood Pressure

Refer to page 18 for measurement with the desired systolic blood pressure.


6. User Selection

Press the **SET** button before measuring blood pressure to select a user from 1 to 4.

In standby, press the **SET** button.

Each time the **SET** button is pressed, the user changes.


Press the **START** button to set to the currently displayed user.

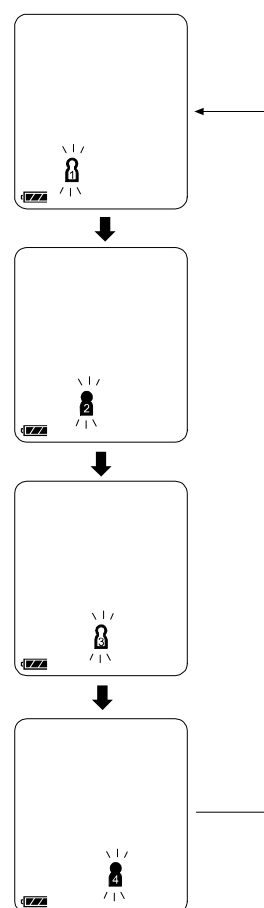

Using the Monitor

Inserting / Changing the Batteries

1. Remove the battery cover.
2. Remove the used batteries and insert new batteries into the battery compartment as shown, making sure that the polarities (+) and (-) are correct.
Use only R6P, LR6 or AA batteries.
3. Putting on the battery cover.

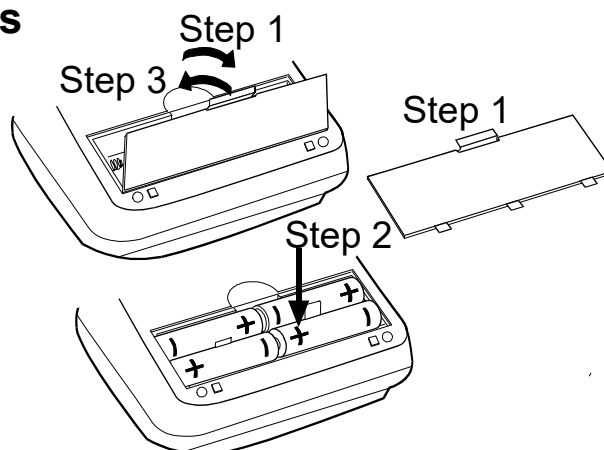


CAUTION

- ☐ Insert the batteries as shown in the battery compartment. If inserted incorrectly, the device will not work.
- ☐ When  (LOW BATTERY mark) blinks on the display, replace all batteries with new ones. Do not mix old and new batteries. It may shorten the battery life, or cause the device to malfunction.
After the device turns off, wait a few seconds before replacing the batteries. If  (LOW BATTERY mark) appears even after the batteries are replaced, take a blood pressure measurement. The device may then recognize the new batteries.
- ☐  (LOW BATTERY mark) does not appear when the batteries are drained.
- ☐ The battery life varies with the ambient temperature and may become shorter at low temperatures. Generally, four new LR6 batteries will last approximately for one year when used twice for measurement each day.
- ☐ Use the specified batteries only.
- ☐ Remove the batteries if the device is not to be used for a long time. The batteries may cause leakage and operational issues.

Using the Monitor

Connecting the Air Hose


Insert the air connector plug into the air socket firmly.

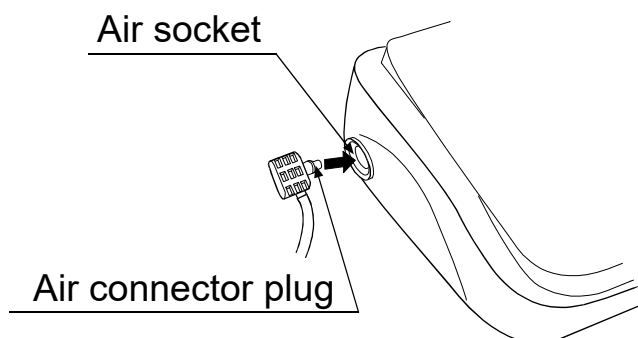

Connecting the AC Adapter

Insert the AC adapter plug into the DC jack.

Then, connect the AC adapter to an electrical outlet.

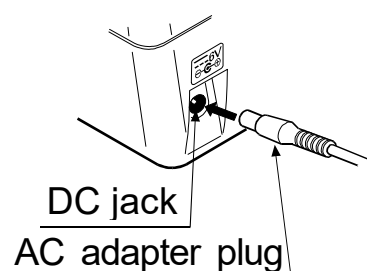

- ☐ Use the specified AC adapter.
(Refer to page 25.)
- ☐ When disconnecting the AC adapter from the electrical outlet, hold and pull the AC adapter body out of the outlet.
- ☐ When disconnecting the AC adapter plug from the blood pressure monitor, hold and pull the AC adapter plug out of the monitor.

Using the Monitor

Adjusting the Built-in Clock

Adjust the clock prior to use.

1. Press and hold the **[SET]** button until the year starts blinking.
 2. Select the year using the **▲** or **▼** button. Press the **[SET]** button to set the current year and move to month/day selection. The date can be set anywhere between the years 2013 and 2059.
 3. Select the month using the **▲** or **▼** button. Press the **[SET]** button to set the current month and move to day selection.
 4. Select the day using the **▲** or **▼** button. Press the **[SET]** button to set the current day and move to hour/minute selection.
 5. Select the hour using the **▲** or **▼** button. Press the **[SET]** button to set the current hour and move to minute selection.
 6. Select the minute using the **▲** or **▼** button. Press the **[START]** or **[SET]** button to turn the device off.
- ☐ Holding down the **▲** or **▼** button will change the value continuously.

Note: After three minutes of non-operation, the device will be turned off automatically.


When the clock has not been set, the clock display indicates dashes as shown to the right.

- / - -
- : - -

When using the device for the first time, the clock is not adjusted.

When the device is disconnected from the power supply, the set date and time will be deleted.

When this happens, please set again.

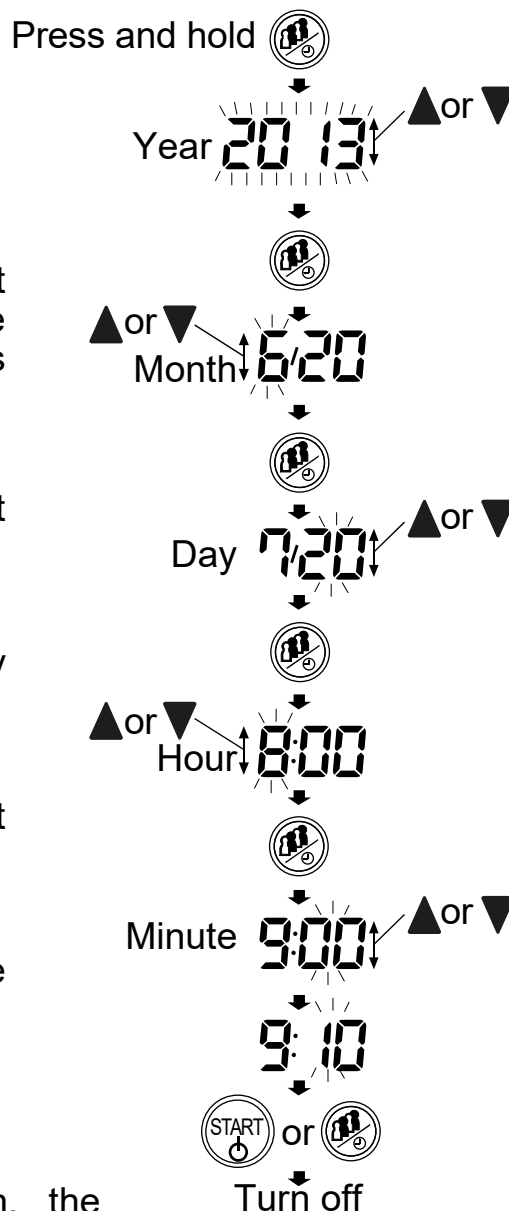

Pressing the **[START]** button will turn the device off anytime.

Using the Monitor

Selecting the Correct Cuff Size

Using the correct cuff size is important for an accurate reading. If the cuff is not the proper size, an incorrect blood pressure value may be displayed.

- ☐ The arm size is printed on each cuff.
- ☐ The index ▲ and proper fit range, on the cuff, tell you if you are applying the correct cuff. (Refer to Table "Symbols that are printed on the cuff" on the next page)
- ☐ If the index ▲ points outside of the range, contact your local dealer to purchase a replacement cuff.
- ☐ The arm cuff is a consumable. If it becomes worn, purchase a new one.


Arm Size	Recommended Cuff Size	Catalog Number
31 cm to 45 cm	Large Adult cuff	CUF-D-LA-ISO
22 cm to 42 cm	Wide range cuff	CUF-I-ISO
22 cm to 32 cm	Adult cuff	CUF-F-A-ISO

Arm size: The circumference of an upper arm.

Note: The UA-767F is not designed for using a small cuff.

Applying the Arm Cuff


1. Wrap the cuff around the upper arm, about 1 to 2 cm above the inside of the elbow, as shown.
Apply the cuff directly against the skin, as clothing may cause a faint pulse, and result in a measurement error.
2. Constriction of the upper arm, caused by tightly rolling up a shirtsleeve, may cause inaccurate readings.
3. Confirm that the index ▲ points within the proper fit range.

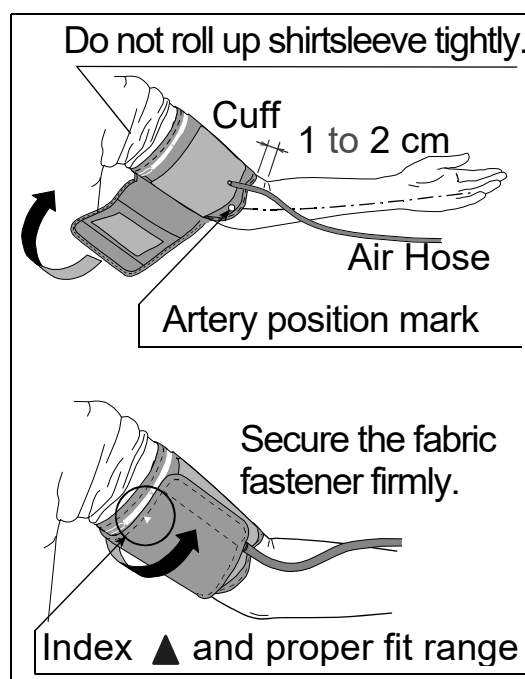

Using the Monitor

Symbols that are printed on the cuff

Symbols	Function / Meaning	Recommended Action
●	Artery position mark	Set the ● mark on the artery of the upper arm or in line with the ring finger on the inside of the arm.
▲	Index	_____
REF	Catalog number	_____
A	Proper fit range for the adult cuff. It's printed on the adult cuff.	_____
L	Over range printed on the adult cuff and wide range cuff.	Use the large adult cuff instead of the adult cuff or wide range cuff.
W	Proper fit range for the wide range cuff. It's printed on the wide range cuff.	_____
L	Proper fit range for the large adult cuff. It's printed on the large adult cuff.	_____
S	Under range printed on the adult cuff and wide range cuff.	_____
A	Under range printed on the large adult cuff.	Use the adult cuff instead of the large adult cuff.
LOT	Lot number	_____

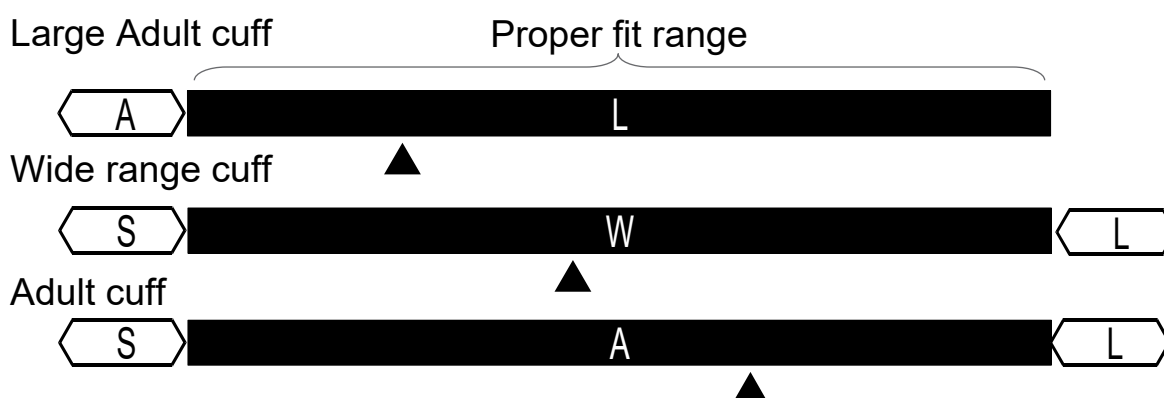

Using the Monitor

How to Take Accurate Measurements

For the most accurate blood pressure measurement:

- ☐ Sit comfortably on a chair. Place your arm on the table. Do not cross your legs. Keep your feet flat on the floor and straighten your back.
- ☐ Relax for about five to ten minutes before taking the measurement.
- ☐ Place the arm at center of the cuff and keep the arm at the same level as your heart.
- ☐ Remain still and keep quiet during the measurement.
- ☐ Do not measure right after physical exercise or a bath. Rest for twenty or thirty minutes before taking the measurement.
- ☐ Try to measure your blood pressure at the same time every day.

Measurement

During the measurement, it is normal for users to feel tight. (Do not be alarmed).

After Measurement

After measurement, press the START button to turn the device off.



Remove the cuff and the readings will be recorded. After one minute of non-operation, the device will be turned off automatically.

Measurements

Before measurement, read the section “Notes for Accurate Measurement” on the next page.

Normal Measurement

1. Press the **SET** button to select a user from 1 to 4.

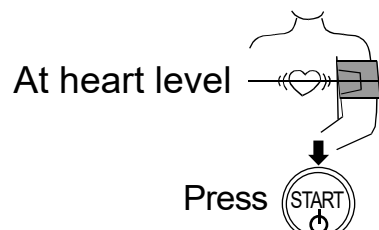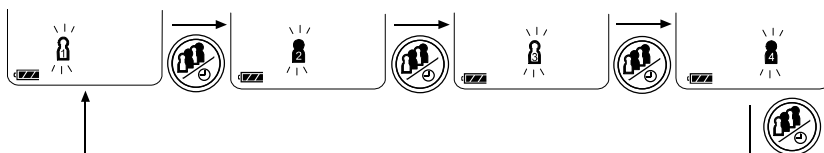

2. Apply the cuff on the arm (preferably the left arm).
Sit quietly during the measurement.

3. Press the **START** button.
All of the display segments are displayed.
Zero (0) is displayed blinking briefly.
The display changes, as indicated in the figure at the right, as the measurement begins. The cuff starts to inflate. It is normal for the users to feel tight. A pressure bar indicator is displayed, on the left edge of the display, during the inflation.

Note: If you want to stop inflation at any time, press the **START** button again.


4. When inflation is completed, deflation starts automatically and ♥ (heart mark) blinks, indicating that the measurement is in progress. Once the pulse is detected, the mark blinks with each pulse beat.

Note: If an appropriate pressure is not obtained, the device starts to inflate again automatically.
To avoid re-inflation, see the section “Measurement with the Desired Systolic Blood Pressure” on the next page.


5. When the measurement is completed, the systolic and diastolic blood pressure readings and pulse rate are displayed. The cuff exhausts the remaining air and deflates completely.
6. When not recording the measurement data, press the ▲ or ▼ button.
7. Press the **START** button to turn the device off. After one minute of non-operation, the device will be turned off automatically.

Note: Allow at least three minutes between measurements on the same person.


All of the display segments displayed




Zero display
Starts inflation



Pressurizing



Measurement
in progress




Systolic blood pressure

Diastolic blood pressure

WHO classification

Pulse rate



Exhausts remaining
air automatically


Measurements

Measurement with the Desired Systolic Blood Pressure

The UA-767F is designed to detect the pulse and to inflate the cuff to a systolic blood pressure level automatically.

Use this method when re-inflation occurs repeatedly or when the results are not displayed even if the pressure decreases to 20 mmHg or less.

1. Apply the cuff on the arm at heart level (preferably the left arm).
2. Press and hold the **START** button until a number about 30 to 40 mmHg higher than your expected systolic blood pressure appears.
3. When the desired number is reached, release the **START** button to start measurement. Continue to measure your blood pressure as described on the previous page.

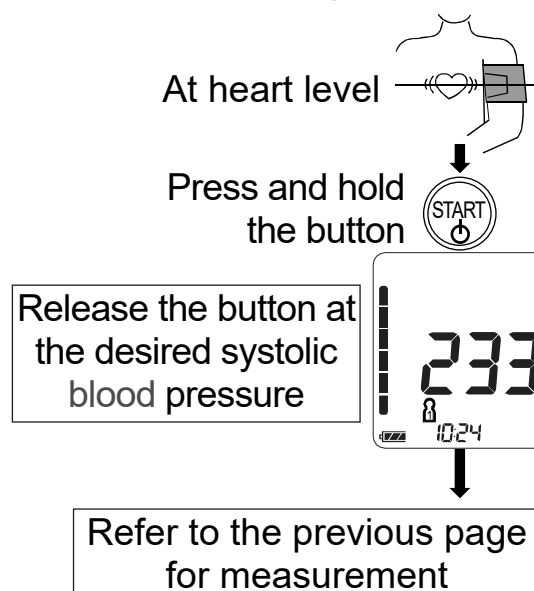

Notes for Accurate Measurement

- ☐ Sit down in a comfortable position. Place your arm on a table with your palm facing upward and the cuff at the same level as your heart.
- ☐ Relax for about five to ten minutes before taking the measurement. If you are excited or depressed by emotional stress, the blood pressure reading may be higher (or lower) than a normal blood pressure reading and the pulse rate will usually be faster than normal.
- ☐ An individual's blood pressure varies constantly, depending on what you are doing and what you have eaten. What you drink may have a strong and rapid effect on your blood pressure.
- ☐ This device bases its measurements on the heartbeat. If you have a weak or irregular heartbeat, the device may have difficulties determining your blood pressure.
- ☐ If the device detects a condition that is abnormal, it will stop the measurement and the error symbol will be displayed. Refer to pages 7 and 8 for the description of symbols.
- ☐ This blood pressure monitor is intended for use by people 13 years and older.
- ☐ The automatic blood pressure monitor's performance may be affected by excessive temperature or humidity, or altitude.

Recalling the Memory Data

Note: This device stores the last 60 measurements for each of the four users in memory.

1. Press the ▲ or ▼ button.
The average of all measurements and the number of data are displayed.
(If no data, "0" is displayed. Press the ▲, ▼ or [START] button to turn the device off.)

2. Each time the ▼ button (or the ▲ button to display the data in the reverse order) is pressed, the memory data is displayed as follows.

Most recent data (No.n, in the example, No.35)

Three seconds after the data number display, the measurement data is displayed.




Last data (No.1)


Three seconds after the data number display, the measurement data is displayed.

3. After the last data is displayed, press the ▼ button to return the average display of all measurements.

Press ▲ or ▼

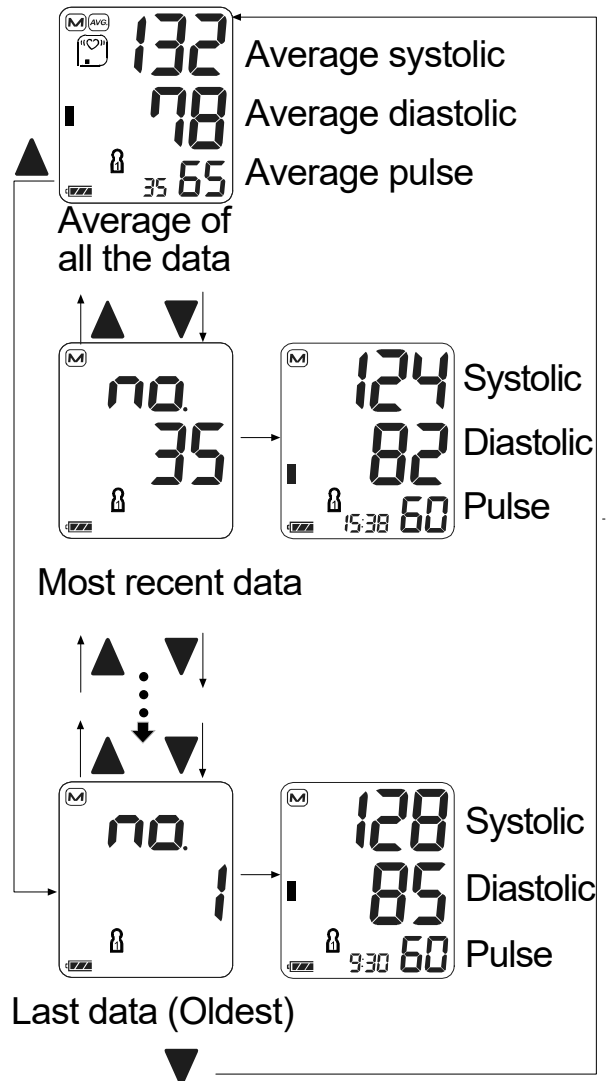

4. Press the **SET** button to display the memory display after changing the user number.
5. Press the **START** button to turn the device off. After one minute of non-operation, the device will be turned off automatically.

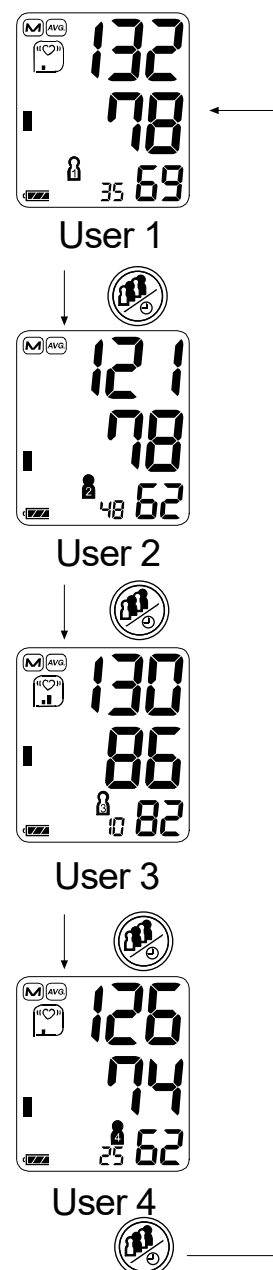

What Is the IHB/AFib Indicator?

When the monitor detects an irregular rhythm during the measurements, the IHB/AFib indicator will appear on the display with the measurement values.

Note: We recommend contacting your physician if you see this «♥» IHB/AFib indicator frequently.

What Is the AFib?

The heart contracts due to electrical signals occurring in heart and sends blood through the body. Atrial fibrillation (AFib) occurs when the electrical signal in the atrium becomes confused and leads to disturbances in the pulse interval. AFib can cause blood to stagnate in the heart, which can easily create clots of blood, a cause of stroke and heart attack.

%IHB/AFib

%IHB/AFib is displayed as frequency of IHB/AFib detected.

IHB/AFib can detect not only noises such as physical movement but also an irregular heartbeat. Therefore, we recommend contacting your physician if %IHB/AFib level is high.


$$\%IHB/AFib = \frac{\left(\begin{array}{c} \text{Number of detected} \\ \text{IHB/AFibs in memory} \end{array} \right)}{\left(\begin{array}{c} \text{Total number} \end{array} \right)} \times 100 [\%]$$

Display of %IHB/AFib: %IHB/AFib is displayed when displaying average values.

(Refer to “2. Recalling the Data” in “Operation Mode”)

%IHB/AFib is not displayed when the memory number is six or less.


Average value display



Level 0 %IHB/AFib=0	Level 1 %IHB/AFib=1 - 9	Level 2 %IHB/AFib=10 - 24	Level 3 %IHB/AFib=25 - 100
Not displayed	«♥»	«♥»	«♥»

Pressure Bar Indicator


The indicator monitors the progress of the pressure during the measurement.

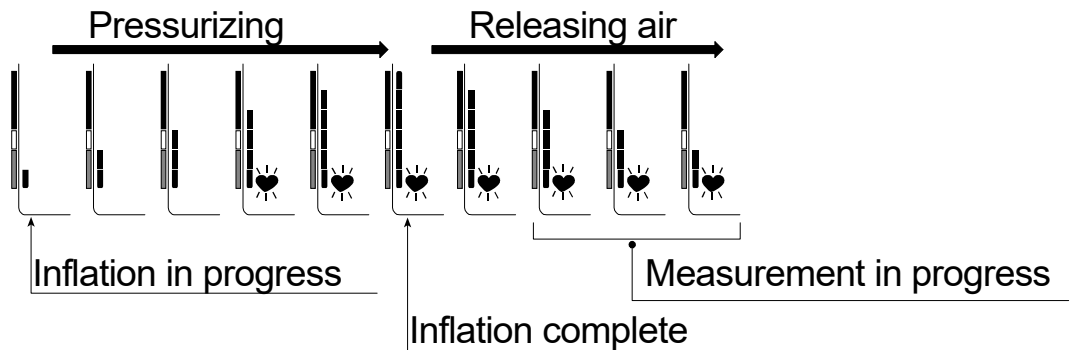

WHO Classification Indicator


Each segment of the bar indicator corresponds to the WHO blood pressure classification is described on the next page.

WHO Classification Indicator

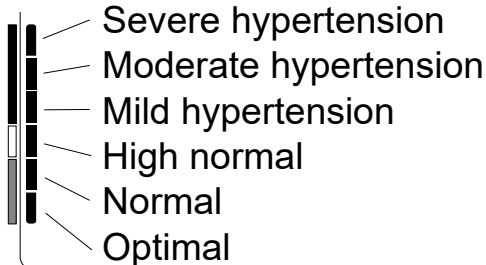

■ : The indicator displays a segment, based on the current data, corresponding to the WHO classification.

Example:



Moderate hypertension



Mild hypertension



High normal

About Blood Pressure

What is Blood Pressure?

Blood pressure is the force exerted by blood against the walls of the arteries. Systolic blood pressure occurs when the heart contracts. Diastolic blood pressure occurs when the heart expands. Blood pressure is measured in millimeters of mercury (mmHg). One's natural blood pressure is represented by the fundamental pressure, which is measured first thing in the morning while one is still at rest and before eating.

What is Hypertension and How is it Controlled?

Hypertension, an abnormally high arterial blood pressure, if left untreated, may cause many health problems including stroke and heart attack. Hypertension can be controlled by altering lifestyle, avoiding stress, and with medication under a doctor's supervision.

To prevent hypertension or keep it under control:

- ☐ Do not smoke
- ☐ Exercise regularly
- ☐ Reduce salt and fat intake
- ☐ Have regular physical checkups
- ☐ Maintain proper weight


Why Measure Blood Pressure at Home?

Blood pressure measured at a clinic or doctor's office may cause apprehension and may elevate the reading by 25 to 30 mmHg higher than when measured at home. Home measurement reduces the effects of outside influences on blood pressure readings, supplements the doctor's readings and provides a more accurate, complete blood pressure history.

WHO Blood Pressure Classification

Standards to assess high blood pressure, without regard to age, have been established by the World Health Organization (WHO), as shown in the chart.


Reference Material: Journal of Hypertension 1999, Vol 17 No.2

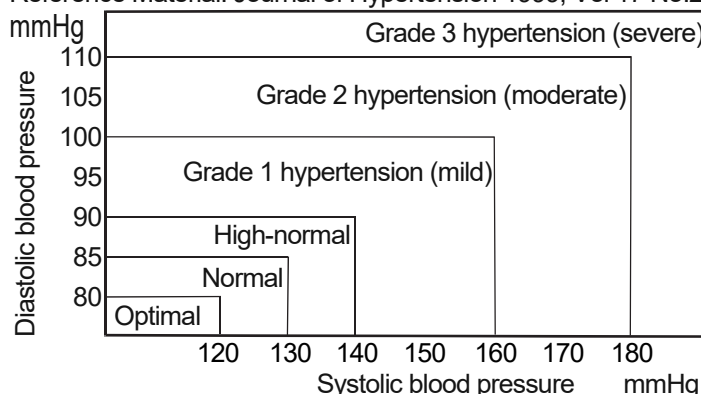

Blood Pressure Variations

An individual's blood pressure varies greatly on a daily and seasonal basis. It may vary by 30 to 50 mmHg due to various conditions during the day. In hypertensive individuals, variations are even more pronounced. Normally, the blood pressure rises when working or playing and falls to its lowest levels during sleep. So, do not be overly concerned by the results of one measurement. Take measurements at the same time every day using the procedure

described in this manual to get to know your normal blood pressure. Regular readings give a more comprehensive blood pressure history. Be sure to note the date and time when recording your blood pressure. Consult your doctor to interpret your blood pressure data.

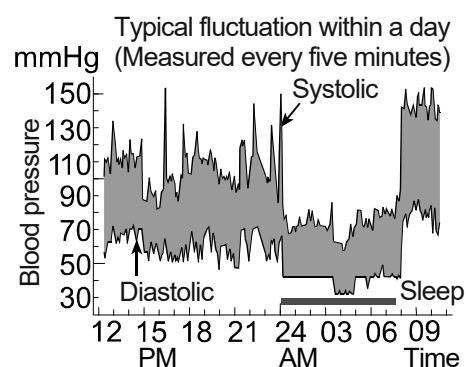

Troubleshooting

Problem	Possible Cause	Suggestion
Nothing appears on the display, even when the power is turned on.	Batteries are drained.	Replace all batteries with new ones.
	Battery terminals are not in the correct position.	Reinstall the batteries with negative and positive terminals matching those indicated on the battery compartment.
The cuff does not inflate.	Battery power is too low.  (LOW BATTERY mark) blinks. If the batteries are drained completely, the mark does not appear.	Replace all batteries with new ones.
The device does not measure. Readings are too high or too low.	The cuff is not applied properly.	Apply the cuff correctly.
	Movement is detected.	Make sure to remain very still and quiet during the measurement.
	The cuff position is not correct.	Sit comfortably and still. Place your arm on a table with your palm facing upward and the cuff at the same level as your heart.
	_____	If you have a very weak or irregular heartbeat, the device may have difficulties in determining your blood pressure.
Other	The value is different from that measured at a clinic or doctor's office.	Refer to the section "Why Measure Blood Pressure at Home?"
	_____	Remove the batteries. Put them back properly and take another measurement.

Note: If the suggestions described above do not solve the problem, contact the authorized dealer. Do not attempt to open or repair this product, otherwise your warranty may be invalid.

Maintenance

Do not open the device. It uses delicate electrical components and an intricate air unit that could be damaged. If you cannot fix the problem using the troubleshooting instructions, contact the authorized dealer in your area or our customer service department. The A&D customer service will provide technical information, spare parts and units to authorized dealers.

The device is designed and manufactured for a long service life. However, it is generally recommended to have the device inspected every 2 years, to ensure proper functioning and accuracy. Please contact the authorized dealer in your area or A&D for maintenance.

Technical Data

Type	UA-767F
Measurement method	Oscillometric measurement
Measurement range	Pressure: 0 - 299 mmHg Systolic blood pressure: 60 - 279 mmHg Diastolic blood pressure: 40 - 200 mmHg Pulse: 40 - 180 beats / minute
Measurement accuracy	Pressure: ± 3 mmHg Pulse: $\pm 5\%$
Power supply	4 x 1.5V batteries (R6P, LR6 or AA) or AC adapter (TB-233C) (Not included)
Number of measurements	Approx. 700 times LR6 (alkaline batteries) Approx. 200 times R6P (manganese batteries) With pressure value 180 mmHg, room temperature 23 °C.
Classification	Internally powered ME equipment (Supplied by batteries) / Class II (Supplied by adapter) Continuous operation mode
Clinical test	According to ISO 81060-2: 2018+A1: 2020 In the clinical validation study, K5 was used on 85 subjects for determination of diastolic blood pressure.
EMD	IEC 60601-1-2: 2014+A1: 2020
Memory	Last 60 measurements for each of the four users
Operating conditions	+10 to +40 °C / 15 to 85 %RH / 800 to 1060 hPa
Transport / Storage conditions	-20 to +60 °C / 10 to 95%RH / 700 to 1060 hPa
Dimensions	Approx. 140 [W] x 60 [H] x 105 [D] mm
Weight	Approx. 255 g, excluding the batteries
Ingress protection	Device: IP20

Applied part	Cuff	Type BF 
Useful life	Device: 5 years (when used six times a day)	
	Cuff: 2 years (when used six times a day)	
	AC adapter: 5 years (when used six times a day)	
Contents *2	1 Blood Pressure Monitor, 1 Instruction Manual, 4 Batteries, 1 Cuff, 1 Carrying case, 1 EMD Technical Documentation	

Accessory AC adapter

The adapter is to connect the device to a power source at home.

TB-233C

Input: AC 100-240V 50/60Hz 0.15A

Output: DC 6V 500mA

Please contact your local A&D dealer for purchasing.

The AC adapter is required to be inspected or replaced periodically.

Symbols that are printed on the AC adapter

Symbols	Function / Meaning
	For indoor use only
	Class II device
	EAC certification device label
	Polarity of AC adapter plug
	Alternating current

Refer to page 6 for the meanings of the other symbols.

Accessories sold separately

Cuff

Catalog Number	Cuff Size	Arm Size
CUF-D-LA-ISO	Large Adult cuff	31 cm to 45 cm
CUF-I-ISO	Wide range cuff	22 cm to 42 cm
CUF-F-A-ISO	Adult cuff	22 cm to 32 cm

Arm size: The circumference of an upper arm.

AC adapter

Catalog Number	Plug (Outlet type)
TB-233C	Type C

*2: Confirm that all of the parts are included to ensure that the medical device is ready to perform safely and as intended.

Note: Specifications are subject to change without prior notice.

IP classification is the degrees of protection provided by enclosures in accordance with IEC 60529. This device is protected against solid foreign objects with a diameter of 12 mm or greater, such as a finger. This device is not protected against water.

[illegible]



 A&D Company, Limited

1-243 Asahi, Kitamoto-shi, Saitama-ken 364-8585 Japan
Telephone: [81] (48) 593-1111 Fax: [81] (48) 593-1119



Emergo Europe B.V.

Westervoortsedijk 60, 6827 AT Arnhem, The Netherlands



A&D INSTRUMENTS LIMITED

Unit 24/26 Blacklands Way, Abingdon Business Park, Abingdon, Oxfordshire, OX14 1DY,
United Kingdom
Telephone: [44] (1235) 550420 Fax: [44] (1235) 550485

A&D Engineering, Inc.

4622 Runway Boulevard, Ann Arbor, MI 48108 USA
Telephone: [1] (888) 726-9966

A&D AUSTRALASIA PTY LTD

32 Dew Street, Thebarton, South Australia 5031, AUSTRALIA
Telephone: [61] (8) 8301-8100 Fax: [61] (8) 8352-7409

ООО A&D RUS

ООО "ЭЙ энд ДИ РУС"

121357, Российская Федерация, г.Москва, ул. Вереysкая, дом 17
(Business-Center "Vereyskaya Plaza-2" 121357, Russian Federation, Moscow, Vereyskaya Street 17)
тел.: [7] (495) 937-33-44 факс: [7] (495) 937-55-66

A&D Technology Trading(Shanghai) Co. Ltd 爱安德技研贸易(上海)有限公司

中国 上海市自由贸易试验区浦东南路855号世界广场32楼C, D室 邮编200120
(32CD, World Plaza, No.855 South Pudong Road, China (Shanghai) Pilot Free Trade Zone,
200120, China)
电话: [86] (21) 3393-2340 传真: [86] (21) 3393-2347

A&D INSTRUMENTS INDIA PRIVATE LIMITED ऐंडडी इन्स्ट्रूमेंट्स इण्डिया प्रा० लिमिटेड

509, उद्योग विहार , फेस -5, गुडगांव - 122016, हरियाणा , भारत
(509, Udyog Vihar, Phase-V, Gurgaon - 122 016, Haryana, India)
फोन : 91-124-4715555 फैक्स : 91-124-4715599

