

UM-102

Digital Sphygmomanometer

Instruction Manual
Manuel d'instructions
Manual de instrucciones
Manuale di Istruzioni
使用手冊

Original
Traduction
Traducción
Traduzione
翻譯

AND
A&D Medical

UM-102

Digital Sphygmomanometer

Instruction Manual

Contents

1.	Dear Customers	2
2.	Preliminary Remarks	3
3.	Contraindications.....	4
4.	Precautions	4
5.	Parts Identification	8
6.	Symbols.....	9
7.	Using the Monitor	11
8.	Measurements.....	15
9.	Useful Features	16
10.	Troubleshooting.....	17
11.	Maintenance	17
12.	Technical Data	19

1. Dear Customers

Thank you for purchasing a state-of-the-art A&D sphygmomanometer. Designed for ease of use and accuracy. We recommend that you read through this manual carefully before using this device for the first time.

Intended User:	This device is designed to be used by people who can measure blood pressure by auscultation.
Applicable Patient:	The device is designed for use on adults and children aged 3 and older.
Environment for Use:	The device is designed for use in a medical facility.
Intended Purpose:	The UM-102 Sphygmomanometer is used by healthcare professionals to determine systolic and diastolic blood pressure, and to measure pulse rate.
Clinical Benefit:	Successful assessment of blood pressure reading in accordance with the device's intended purpose.

Features

Measurement

- This sphygmomanometer is designed to monitor and display cuff pressure during cuff inflation (by rubber bulb) and deflation (by exhaust bulb) while the user determines the patient's blood pressure level by listening for Korotkoff sounds with a stethoscope.

Safety

- This sphygmomanometer is designed to measure a patient's blood pressure without the use of mercury, therefore protecting your local environment.
- An automatic quick exhaust valve is installed in the device to prevent over pressurization of 299mmHg or higher, therefore protecting the patient.

2. Preliminary Remarks

Compliance

- This device conforms to the Medical Device Regulations (EU 2017/745) and UKCA Medical Device Regulations 2002 for Medical Products. This is made evident by the CE2797 and UKCA0086 mark of conformity. (2797 and 0086: The reference numbers to the involved notified body.)
- This device fulfils the following provisions.

 **Medical Device Regulation (EU 2017/745)**

 **UKCA Medical Devices Regulations 2002**

Definitions

SYS	Systolic Blood Pressure
DIA	Diastolic Blood Pressure
PUL	Pulse
Exhaust	This means "releasing the cuff air as soon as possible".
Constant exhaust	This means, "releasing the cuff air at a constant depressurization rate".

Batteries

- Use alkaline batteries (LR6 type, AA type) or equivalent batteries.
- Do not mix new and used batteries.
- Remove the batteries from the device and store them separately if the device will not be used for a month or more. Otherwise, the batteries may degrade.
- The battery life varies with the ambient temperature and may be shorter at low temperatures. Generally, two new LR6 batteries will last approximately for two months when used forty times for measurement each day.

A Defective Sphygmomanometer

- Stop using the device immediately if the device does not work properly. Please attach a note with the following "Do not use this sphygmomanometer" to prevent any further use. This defective device should be stored in a safe place to avoid any misuse until it has been sent for repair.

Repair

- Do not attempt to open the device. Contact your nearest A&D authorized dealer and they will repair or replace the device.
- Do not modify the device. It may cause accidents or damage to the device.

3. Contraindications

- ❑ Do not use the device in an ambulance or air ambulance. Doing so will prevent the device from providing accurate measurements.
- ❑ Do not apply the cuff on an arm with other medical electrical equipment attached. The equipment may not function properly.
- ❑ Do not apply the cuff on an arm with an unhealed wound.
- ❑ Do not apply the cuff on an arm receiving an intravenous drip or blood transfusion. It may cause injury or accidents.
- ❑ Do not use the device where flammable gases such as anesthetic gases are present. It may cause an explosion.
- ❑ Do not use the device in highly concentrated oxygen environments, such as a high-pressure oxygen chamber or an oxygen tent. It may cause a fire or explosion.
- ❑ When the cuff is infected by blood or body fluid, it should be safely disposed of according to local instructions or protocol to avoid any potential spread of infectious disease.
- ❑ People who have a severe circulatory deficit in the arm must consult a doctor before using the device, to avoid medical problems.
- ❑ Do not provide any servicing and perform maintenance while the medical device is in use.
- ❑ Do not use on patients with blood flow disorders.
- ❑ Do not touch the batteries and the patient at the same time. That may result in electrical shock.

4. Precautions

Blood Pressure Measurement

- ❑ The user should stop using the device if there is an abnormality, such as the patient feeling excessive arm pain, and remove the cuff to protect the patient.

Storage

- ❑ Do not store the device where it could be splashed with water or other liquids. The device and cuff are not water resistant. If the device is immersed by accident, it may require servicing. (Do not use the device before it has endured a full service.) Prevent rain, sweat and water from soiling the device and cuff.
- ❑ Do not store the device in a high temperature or high humidity environment, or in direct sunlight.
- ❑ Do not store the device where it could be influenced by vibration or shock.

- ❑ Do not store the device in a dusty, salty or sulfuric environment.
- ❑ Do not store the device where medicines are stored, or where medicines are evaporating.
- ❑ Store the cuff, air hose, and rubber bulb so that they are not bent or blocked. Doing so may cause an accident or damage to the device.

Before Use

- ❑ Make sure that the device works correctly and that measurement values are accurate.
- ❑ Make sure that the cuff and air hoses are properly connected.
- ❑ Check and maintain the cleanliness of the parts in direct contact with the patient.
- ❑ Avoid placing the device near a strong magnetic field or static electricity.
- ❑ Avoid placing the device near high frequency surgical equipment.
- ❑ When reusing the device, confirm that the device is clean.
- ❑ Allow the device to adapt to the surrounding environment before use (about one hour).

During Use

- ❑ This device was not designed for patients' own use so care must be taken to ensure accurate results and to avoid possible accidents.
- ❑ Regularly confirm patient status when measurement is performed frequently or for a long time. Otherwise, damage may be caused due to peripheral arterial disease.
- ❑ Stop using the device immediately, if the patient feels pain during the measurement or if the device does not work properly.
- ❑ Stop using the device if you notice any abnormalities (for example; liquid inside the device) and request a full service.
- ❑ To measure blood pressure, the arm must be squeezed by the cuff hard enough to temporarily stop blood flow through the artery. This may cause pain, numbness or a temporary red mark to the arm. This condition will appear especially when measurement is repeated successively. Any pain, numbness, or red marks will disappear with time.
- ❑ This is a device which needs to handle with care. Strong impact may result in malfunction of the device.
- ❑ Be careful not to get hurt when handling the damaged device.
- ❑ Do not replace the batteries during use of the device.
- ❑ Do not touch the batteries and the patient at the same time.
- ❑ Should the batteries short-circuit, they may become hot and potentially cause malfunctions and scalding.
- ❑ Use the device so that the air hose is not bent or blocked. Using the cuff with the air hose kinked or bent may result in peripheral circulatory failure due to hemostasis in the arm (caused by air remaining in the cuff).
- ❑ Measurements may be distorted if the device is used close to televisions, microwave ovens, cellular telephones, X-ray or other devices with strong

electrical fields.

- ❑ Wireless communication devices, such as home networking devices, mobile phones, cordless phones and their base stations, and walkie-talkies can affect this digital sphygmomanometer.

After Use

- ❑ Clean the device, cuff and accessories with a dry, soft cloth or a wet cloth with water or a neutral detergent. Do not pull or kink the hoses. Do not use any organic solvent, (antiseptic solution or other harsh chemicals) to clean the device, cuff or accessories.
- ❑ Press  button to turn off the power after measurement.
- ❑ Keep the original box for further transportation after purchasing the device.
- ❑ Be careful not to get your fingers caught when folding the device.

Periodic Maintenance

- ❑ This device is a precision instrument and contains electronic circuitry. Please check all functions periodically. Contact your nearest A&D authorized dealer for official calibration/check-up, according to your local regulations.
- ❑ Used equipment, parts and batteries are not treated as ordinary household waste, and must be disposed of according to the applicable local regulations.
- ❑ The user authority (the hospital, clinic, etc.) is responsible for the safe use and maintenance of this electronic medical device. Care should be taken to follow the specified daily maintenance and inspection procedures for safe use.

How to Take Proper Measurements

For the most accurate blood pressure measurement:

- ❑ Confirm that a patient does not cross the legs, patient's legs touch on the floor and patient's back and arms are supported.
- ❑ Let a patient relax for about five to ten minutes before measurement.
- ❑ Place the center of the cuff at the same height as a patient's heart.
- ❑ A patient must remain still and keep quiet during the measurement.
- ❑ Do not measure right after exercising or taking a bath. A patient must rest for twenty to thirty minutes before the measurement.

Notes for Proper Measurement

- ❑ Let a patient sit down in a comfortable position. Confirm that the patient does not cross their legs, that their feet touch the floor (if possible), and that their back and the arm being measured are supported.
- ❑ Let a patient relax for about five to ten minutes before taking a measurement. If a patient is excited or depressed by emotional stress, the measurement will reflect this stress as a higher (or lower) than a normal blood pressure reading and the pulse reading will usually be faster than normal.

- ❑ An individual's blood pressure varies constantly, depending on what a patient is doing and what a patient has eaten. What a patient drinks can have a very strong and rapid effect on patient's blood pressure.
- ❑ Should the device detect a condition that is abnormal, it will stop the measurement and display an error symbol. Refer to page 9 for the description of symbols.
- ❑ Measurement may be affected by the position of the cuff, as well as the patient's posture (standing, sitting, supine), movement, or physiological condition.
- ❑ Measuring blood pressure too frequently may cause harm due to blood flow interference. Check that the operation of the device does not result in prolonged impairment of blood circulation, when using the device repeatedly.
- ❑ Use of accessories not detailed in this manual may compromise safety.

For the auscultation measurement

- ❑ K5 is recommended for the auscultation measurement in adults.
- ❑ K4 is recommended for the auscultation measurement in children aged 3 to 12 years.
- ❑ K5 is recommended for the auscultation measurement in pregnant women, however, K4 should be used if the sounds can be heard even with the cuff deflated.
- ❑ During the auscultation measurement, the operator should be in a position where the pressure value is clearly visible

Note: K5 is the point at which the Korotkoff sounds can no longer be heard.


K4 is the point at which the Korotkoff sounds changed in the tones heard through a stethoscope from a clear tapping sound to a muffled sound.

Other

- ❑ This sphygmomanometer is intended for adults and children aged 3 and older. Do not use this device on newborns or infants.
- ❑ If you have had a mastectomy or lymph node clearance, please consult a doctor before using the device.
- ❑ Do not let children use the device by themselves and do not use the device in a place within the reach of infants. It may cause accidents or damage.
- ❑ Do not inflate without wrapping the cuff around the upper arm.
- ❑ When any serious incident occurs in relation to this device, report to its manufacturer and the competent authority in your country.
- ❑ Confirm for proper operation before use, if the packaging is damaged, unintentionally opened and exposed to environmental conditions outside of those specified.


5. Parts Identification

Main Body and Accessories

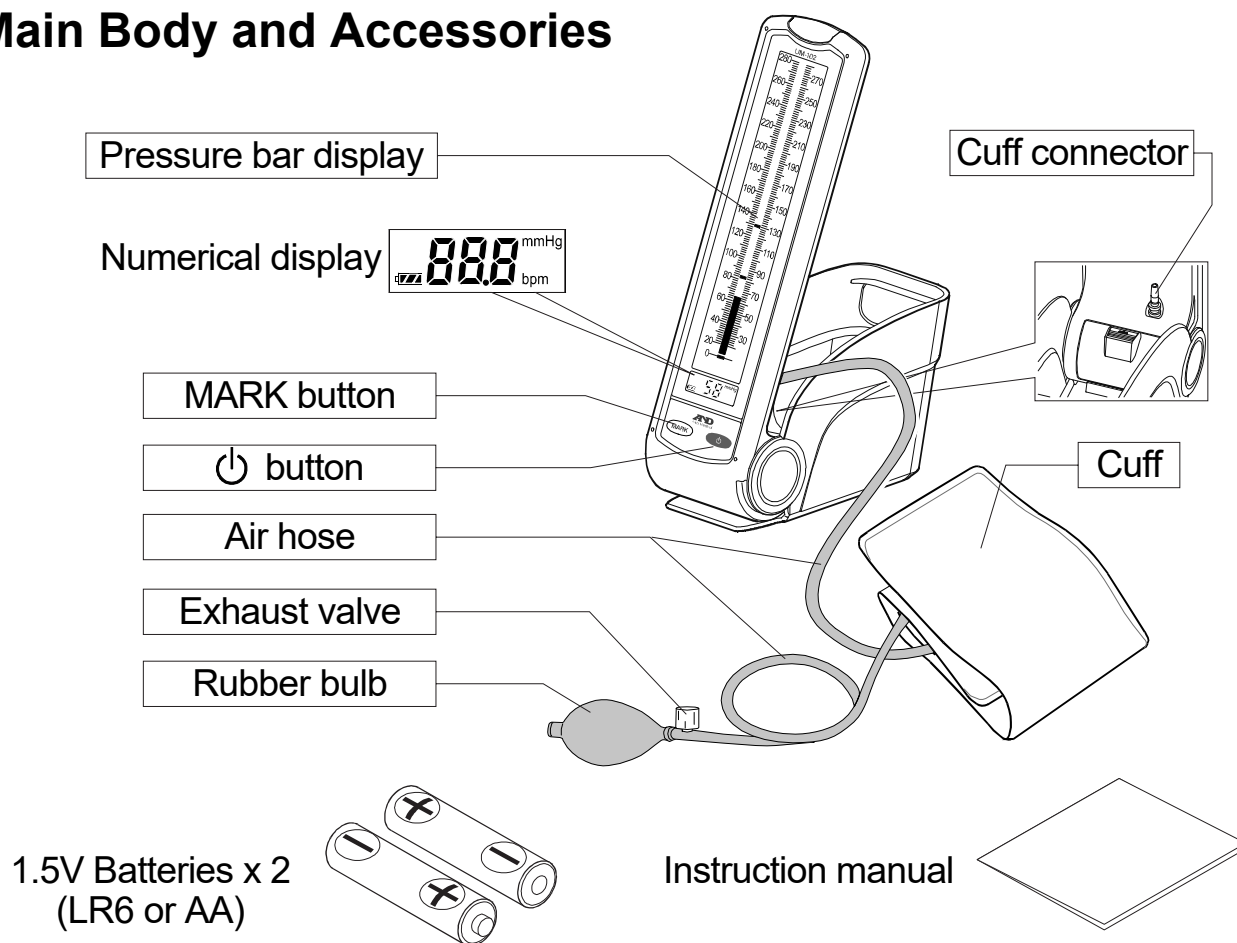



	Function
Power Button	Turns on the device and start / stop measurement.
MARK button	During the measurement..... Puts a marker at a pressure value After turned off..... Indicates a lifetime counter
Numerical display	During the measurement..... Indicates pressure value After exhausted air..... Indicates pulse rate

Display

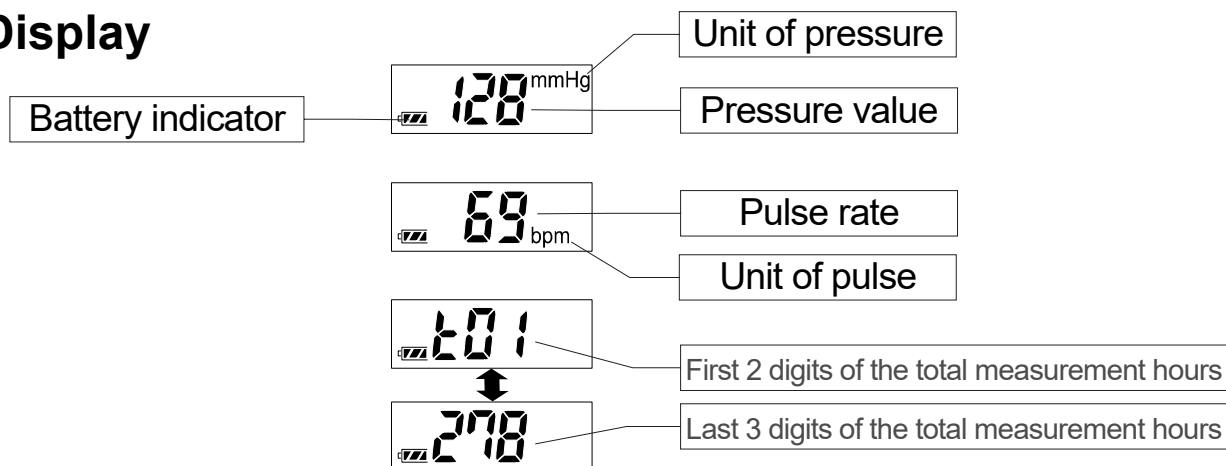

6. Symbols

Symbols	Function / Meaning	Recommended Action
	Press  to turn on the device. Press  during measurement to enter standby.	—
MARK	Pressure value holding and lifetime counter	—
	Battery installation guide	—
	Serial Number	—
	Unique Device Identifier	—
2023 	Date of manufacture	—
	Type BF applied part	—
	Full Battery The battery power indicator during the measurement.	—
	Low Battery The battery is low when it blinks.	Replace all batteries with new ones, when the indicator blinks.
Er 1	Pressure remains in the cuff.	Exhaust it with the exhaust valve.
Er 2	Measurement overtime	
Er 3	Device is out of order.	Send for service.
Err	The pulse is not detected correctly.	Take another measurement.
mmHg	Unit of pressure	—
bpm	Unit of pulse	—
	CE marking	—
	WEEE label	—
	Manufacturer	—
	European Authorized Representative	—


Symbols	Function / Meaning	Recommended Action
	Refer to instruction manual/booklet *1	—
	Warning; Hot surface	—
	UK Conformity Assessed marking	—
	UK Responsible Person	—
	Medical Device	—
	Keep dry	—
	Temperature limitation	—
	Humidity limitation	—
	Atmospheric pressure limitation	—
	EU Importer	—
	UK Importer	—

*1 The symbol color: Blue

7. Using the Monitor

Inserting / Changing the Batteries

1. Remove the battery cover.
2. Insert a new set of batteries into the battery compartment as shown. Make sure the polarities (+) and (-) are correct. Use only LR6, AA or equivalent batteries.
3. Putting on the battery cover.

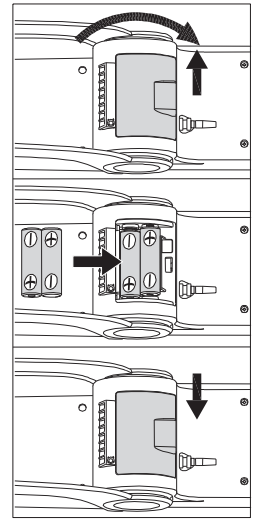


CAUTION

- ❑ Insert the batteries in the battery compartment.
If not, the device will not work.
- ❑ When  (LOW BATTERY mark) blinks in the LCD display, replace all batteries with new ones. Do not mix old and new batteries. It may shorten the battery life, or cause the device to malfunction.
- ❑ The battery life varies with the ambient temperature and may become shorter at low temperatures.
- ❑ Use the specified batteries only. The batteries provided with the device are for testing and may have a limited life.
- ❑ Remove the batteries if the device will not be in use for a prolonged period of time as the batteries may leak and cause a device malfunction.

Connecting the Air Hose

Insert the air hose into the cuff connector firmly.

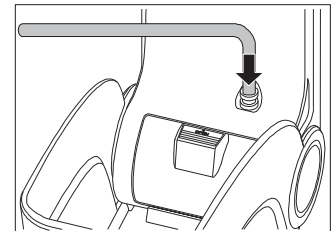

Connecting the Connector and Plug for the Cuff

(Sold separately)



1. Insert the air hose socket into the cuff connector.

2. Insert the air hose plug to the air hose of the cuff.

3. Connect the air hose plug of the cuff to the air hose socket of the main body.


Securely connect by turning the air hose plug the direction of the arrow.

□ Use the specified connector. (Refer to page 20)

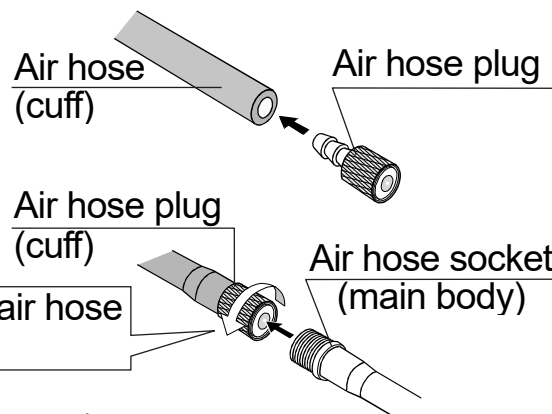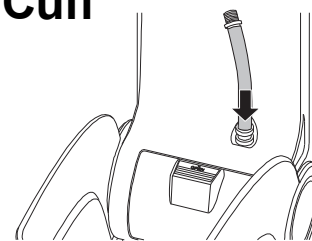

Installing the Device to Mobile Stand (Sold separately)

Install the device with the included four screws to mobile stand.

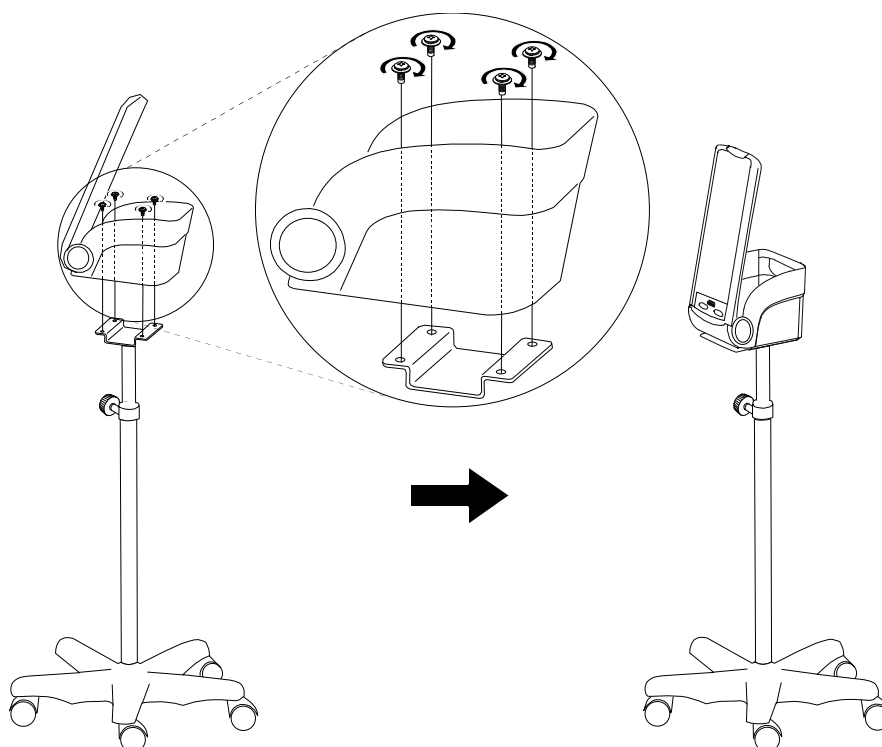

Selecting the Proper Cuff

Using the correct cuff size is important for accurate readings. If the cuff is not the proper size, an incorrect blood pressure value may be displayed.


- The INDEX and RANGE markings on the cuff will indicate that you are using the proper cuff or not. (Refer to "**Attaching the Arm Cuff**" in the next section)

Arm Size	Cuff Size	Catalog Number
41 cm to 50 cm	LL Cuff	CUF-KW-LL
31 cm to 45 cm	Large Adult Cuff	CUF-KW-LA
22 cm to 32 cm	Adult Cuff	CUF-KW-A
16 cm to 24 cm	Small Adult Cuff	CUF-KW-SA
12 cm to 17 cm	SS Cuff	CUF-KW-SS

Arm size: The circumference of an upper arm.

Attaching the Arm Cuff

1. Wrap the cuff around the upper arm, about 1 to 2 cm above the elbow as shown on the right. Apply the cuff directly against the skin, as clothing may cause a faint pulse and could result in a measurement error.
2. Constriction of the upper arm, caused by rolling up a shirtsleeve, may interfere with accurate readings.
3. Make sure that the index points are within the range.

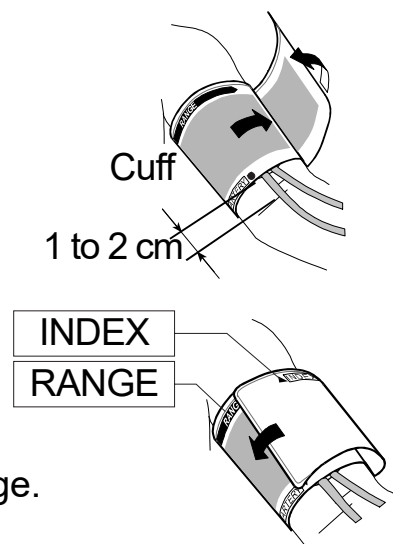

Symbols that are printed on the cuff

Symbols	Function / Meaning
▲ INDEX	Proper fit range
RANGE	
ARTERY ●	Artery position mark
THIS SIDE TO PATIENT	Instructions to the patient
REF	Catalog number
LOT	Lot number
ADULT	Cuff size 22 cm to 32 cm
LL	Cuff size 41 cm to 50 cm
LARGE ADULT	Cuff size 31 cm to 45 cm
SMALL ADULT	Cuff size 16 cm to 24 cm
SS	Cuff size 12 cm to 17 cm
⚠	Means the symbol for suggestions on operation
CE	CE marking
LATEX	Latex free
📖	Refer to instruction manual/booklet *1
	Cuff Wrap position


*1 The symbol color: Blue


8. Measurements

1. Apply the cuff on the arm (preferably the left arm).
Keep the patient still during the measurement.



2. Press the  button.

- ☐ When the  button is pressed, all of the display symbols will appear for about one second.
- ☐ When  starts flashing, the device is ready for measurement. If air is remaining in the cuff when the  button is pressed, the display will indicate an error code .



Turn the device off (press the  button again) and turn the exhaust valve counterclockwise once to release all the air in the cuff. Then press the  button again to reactivate the device.

3. Place the stethoscope on the brachial artery and pressurize the cuff by squeezing the rubber bulb. (Make sure the exhaust valve is completely closed.)
 - ☐ While the cuff is inflating, the pressure bar will move and in turn the LCD will display a number indicating the pressure.
 - ☐ Inflate the cuff to 30 to 40 mmHg higher than the patient's usual systolic value.

Note: If you want to stop inflation at any time, press either the  button or turn the screw of the exhaust valve to release the air.

4. When inflation is completed.
 - ☐ Turn the exhaust valve screw to release air slowly.
 - ☐ Measure the systolic blood pressure and the diastolic blood pressure by stethoscope.
5. The heart rate is shown on the numerical display when the measurement is complete or meets the following conditions.
 - ☐ When you pressurize 80mmHg or higher for the measurement.
 - ☐ When the pressure drops to 20mmHg or lower.


6. Turn the exhaust valve screw counterclockwise to release all the air from the cuff.

- ❑ If a measurement is taken with insufficient pressure, the --- mark will be displayed. Re-pressurize the cuff to a pressure that is about 30 to 40 mmHg higher than the previous attempt.
- ❑ An error message Err will be displayed if a measurement is taken with insufficient pulses or in a very noisy environment.

7. Press the ⏻ button again to turn off the power.

Note: Model UM-102 has an automatic power-off function.


Allow at least three minutes between measurements on the same person.

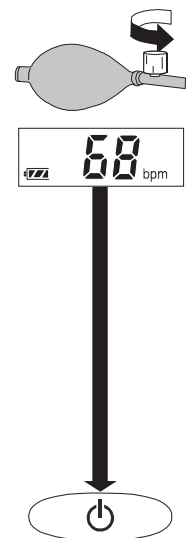

9. Useful Features

Measurement with MARK Button


You can put a marker at a certain pressure value when the MARK button is pressed during the measurement process. Up to 5 markings can be shown over the range of 40mmHg.

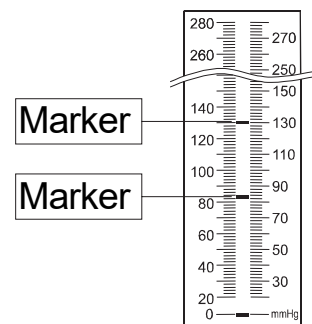

Lifetime Counter

When the MARK button is pressed while the device is off, the lifetime counter is displayed.

This counter function indicates the hours the device was in use and helps to determine when maintenance is necessary. High digits and Low digits are alternatively displayed. The example indicates that the device has been in use for 1,278 hours.

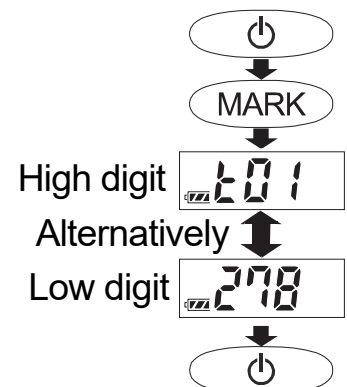

10. Troubleshooting

Problem	Possible Cause	Suggestion
Nothing appears in the display, even when the power is turned on.	Batteries are empty.	Replace all batteries with new ones.
	Battery polarities are not in the correct position.	Reinstall the batteries with the negative and positive ends matching those indicated in the battery compartment.
The cuff is not inflated.	The cuff is not connected properly.	Check the twist of the air hose, and connection of the cuff and air hose.
	There is leakage of air from the cuff or rubber bulb.	Replace the cuff or rubber bulb with a new one.
Remain a display of 	Error symbol is displayed one minute later.	Refer to "6. Symbols".

Note: If the suggestions described above do not solve the problem, contact the authorized dealer. Do not attempt to open or repair this product, otherwise your warranty may be invalid.

11. Maintenance

Do not attempt to open the device as the delicate electrical components and intricate air unit inside could be damaged. If you cannot solve the problem using our troubleshooting guide, request assistance from your authorized dealer or from any A&D service group.

The device is designed and manufactured for a long service life. However, it is generally recommended to have the device inspected every 2 years, to ensure proper functioning and accuracy. Please contact either your authorized dealer or A&D for maintenance.

CAUTION


- ☐ The sphygmomanometer is not waterproof device. Do not splash water on it and avoid exposure to moisture.
- ☐ Do not use a organic solvent such as thinner or benzine.
- ☐ The sphygmomanometer cannot be sterilized by autoclave, EOG or formaldehyde etc.

Cleaning

- ❑ When cleaning the device and cuff, turn off the power by pressing  button and remove the batteries.
- ❑ When the main body or cuff is dirty, wipe them fully by using a gauze or cloth dampened with water or warm water avoiding excess water.
- ❑ To prevent a risk due to infection, disinfect the main body and cuff regularly. When disinfecting them, wipe them gently by using the gauze or dampened cloth with local antiseptic solution then wipe the moisture off the surface by using a dry soft cloth.
- ❑ Use the following disinfectants to clean the main body and cuff.

Ethanol (70%)
Isopropanol (70%)
Chlorhexidine Gluconate Solution (0.5%)
Benzalkonium Chloride Solution (0.05%)
Sodium Hypochlorite (0.05%)

- ❑ Do not wipe off the valve and its vicinity with gauze soaked in disinfectant solution. It will cause stuffing of the rubber bulb.
- ❑ Clean the device about once every month, based on the policy or instruction specified by the user authority.

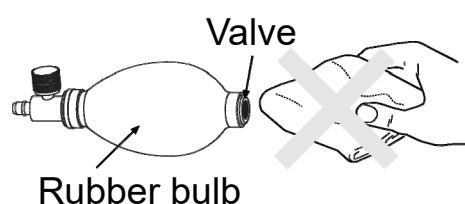

Disposal

This unit and its batteries are not treated as ordinary household waste and must be disposed of according to the applicable local regulations.


Item	Parts	Material
Package	Box	Cardboard
	Cushion	Cardboard
	Bag	PE
Main unit and accessories	Enclosure	ABS
	Internal parts	General electronic components
	Batteries	Alkaline battery

12. Technical Data

Model	UM-102
Measurement method	By applying pressure, enabling the determination of blood pressure by the auscultatory method.
Measurement range	
Numerical display	Pressure: 0 - 299 mmHg Pulse: 40 - 180 beats / minute
Pressure bar display	Pressure: 20 - 280 mmHg
Measurement accuracy	
Numerical display	Pressure: ± 3 mmHg Pulse: ± 5 %
Power supply	2 x 1.5 V alkaline batteries (LR6 or AA)
Upper arm circumference	22 - 32 cm using the adult cuff
Number of measurements	Approx. 2000 measurements, when AA alkaline batteries are used, with pressure value of 180 mmHg at room temperature of 23°C
Classification	Internally powered ME equipment Continuous operation mode
EMD	IEC 60601-1-2: 2014+A1: 2020
Operating conditions	+10°C to +40°C / 15%RH to 85 %RH 800 hPa to 1060 hPa
Transport / Storage conditions	-20°C to +60°C / 10%RH to 95 %RH 700 hPa to 1060 hPa
Dimensions	Approx. 98 [W] x 326 [H] x 202[D] mm
Weight	Approx. 540 g, excluding batteries
Applied part	Cuff Type BF 
Useful life	Device: 5 years Cuff: 1 year or 30,000 times Rubber bulb unit: 2years
Contents *2	1 Sphygmomanometer, 1 Instruction Manual 2 Batteries, 1 Cuff, 1 Rubber bulb unit 1 Caution instruction


Accessories sold separately

Cuff




Catalog Number	Cuff Size	Arm Size
CUF-KW-LL	LL Cuff	41 cm to 50 cm
CUF-KW-LA	Large Adult Cuff	31 cm to 45 cm
CUF-KW-A	Adult Cuff	22 cm to 32 cm
CUF-KW-SA	Small Adult Cuff	16 cm to 24 cm
CUF-KW-SS	SS Cuff	12 cm to 17 cm

Rubber bulb unit




Catalog Number
UM-102-10

Connector and Plugs for cuff replacement



Catalog Number
UM-102-11

Mobile stand



Catalog Number
UM-ST001

*2: Confirm that all of the parts are included to ensure that the medical device is ready to perform safely and as intended.

Note: Specifications are subject to change without prior notice.

EMD Technical Data Battery-operated Blood Pressure Monitor

Medical Electrical Equipment needs special precautions regarding EMD and needs to be installed and put into service according to the EMD information provided in the following. Portable and mobile RF communication equipment (e.g. cell phones) can affect Medical Electrical Equipment.

The use of accessories and cables other than those specified may result in increased emissions or decreased immunity of the unit.

Table 1 —EMISSION Limits—

Phenomenon	Compliance
Conducted and radiated RF EMISSION CISPR 11	Group 1、Class B

Table 2 —IMMUNITY TEST LEVELS : Enclosure Port—

Phenomenon	IMMUNITY TEST LEVELS
Electrostatic discharge IEC 61000-4-2	±8 kV contact ±2 kV, ±4 kV, ±8 kV, ±15 kV air
Radiated RF EM fields IEC 61000-4-3	10 V/m 80 MHz - 2.7 GHz 80 % AM at 1 kHz
Proximity fields from RF wireless communications equipment IEC 61000-4-3	See table 3
Rated power frequency magnetic fields IEC 61000-4-8	30 A/m 50 Hz or 60 Hz
Proximity magnetic fields IEC 61000-4-39	See table 4

Table 3 —Test specifications for ENCLOSURE PORT IMMUNITY to RF wireless communications equipment—

Test frequency (MHz)	Band (MHz)	Service	Modulation	Maximum power (W)	Distance (m)	IMMUNITY TEST LEVEL (V/m)
385	380 ~ 390	TETRA 400	Pulse modulation 18 Hz	1.8	0.3	27
450	430 ~ 470	GMRS 460 FRS 460	FM ±5 kHz deviation 1 kHz sine	2	0.3	28
710 745 780	704 ~ 787	LTE Band 13,17	Pulse modulation 217 Hz	0.2	0.3	9
810 870 930	800 ~ 960	GSM 800/900 TETRA 800 iDEN 820 CDMA 850 LTE Band 5	Pulse modulation 18 Hz	2	0.3	28
1720 1845 1970	1700 ~ 1990	GSM 1800 CDMA 1900 GSM 1900 DECT LTE Band 1,3,4,25 UMTS	Pulse modulation 217 Hz	2	0.3	28
2450 5240 5500 5785	2400 ~ 2570	Bluetooth WLAN 802.11 b/g/n RFID 2450 LTE Band 7	Pulse modulation 217 Hz	2	0.3	28
	5100 ~ 5800	WLAN 802.11 a/n	Pulse modulation 217 Hz	0.2	0.3	9

Table 4 — Test specifications for ENCLOSURE PORT IMMUNITY to proximity magnetic fields—

Test frequency	Modulation	IMMUNITY TEST LEVEL(A/m)
30 kHz	CW	8
134.2 kHz	Pulse modulation 2.1 kHz	65
13.56 MHz	Pulse modulation 50 kHz	7.5

MEMO

[illegible]



 A&D Company, Limited

1-243 Asahi, Kitamoto-shi, Saitama-ken 364-8585 Japan
Telephone: [81] (48) 593-1111 Fax: [81] (48) 593-1119



Emergo Europe B.V.

Westervoortsedijk 60, 6827 AT Arnhem, The Netherlands



A&D INSTRUMENTS LIMITED

Unit 24/26 Blacklands Way, Abingdon Business Park, Abingdon, Oxfordshire, OX14 1DY,
United Kingdom
Telephone: [44] (1235) 550420 Fax: [44] (1235) 550485

A&D Engineering, Inc.

4622 Runway Boulevard, Ann Arbor, MI 48108 USA
Telephone: [1] (888) 726-9966

A&D AUSTRALASIA PTY LTD

32 Dew Street, Thebarton, South Australia 5031, AUSTRALIA
Telephone: [61] (8) 8301-8100 Fax: [61] (8) 8352-7409

ООО А&Д RUS ООО "ЭЙ энд ДИ РУС"

121357, Российская Федерация, г.Москва, ул. Вереysкая, дом 17
(Business-Center "Vereyskaya Plaza-2" 121357, Russian Federation, Moscow, Vereyskaya Street 17)
тел.: [7] (495) 937-33-44 факс: [7] (495) 937-55-66

A&D Technology Trading (Shanghai) Co. Ltd 爱安德技研贸易(上海)有限公司

中国 上海市自由贸易试验区浦东南路 855 号世界广场 32 楼 C, D 室 邮编 200120
(32CD, World Plaza, No.855 South Pudong Road, China (Shanghai) Pilot Free Trade Zone,
200120, China)
电话: [86] (21) 3393-2340 传真: [86] (21) 3393-2347

A&D INSTRUMENTS INDIA PRIVATE LIMITED ऐ&डी इन्स्ट्रुमेंट्स इण्डिया प्रा० लिमिटेड

509, उद्योग बिहार, फेस -5, गुडगांव - 122016, हरियाणा, भारत
(509, Udyog Vihar, Phase-V, Gurgaon - 122 016, Haryana, India)
फोन : 91-124-4715555 फैक्स : 91-124-4715599

